

BEADBRITE RESEARCH LLC



4811 Lyons Tech Pkwy. Suite 4 Coconut Creek, FL 33073 (954) 426-2360

TECHNICAL NOTE: VITROCOTE™ 10 PARTICLE SIZE ANALYSIS (LOT C7835.2)



LS Particle Size Analyzer

File name: Vitrocote 7835.2 1200 mesh (Control Standard) c.\$02
 Sample ID: Vitrocote 7835.2 1200 mesh (Control Standard) c
 Run number: 2
 Optical model: jbrem-1495-001.rfd PIDS included
 LS 230 VSM+
 Start time: 23:53 4 Nov 2003 Run length: 90 seconds
 Pump speed: 34
 Obscuration: 6% PIDS Obscur: 49%
 Software: 3.01 Firmware: 2.02 0

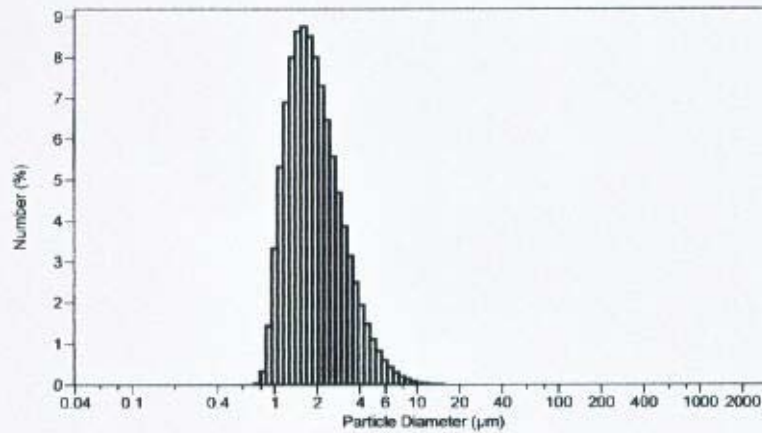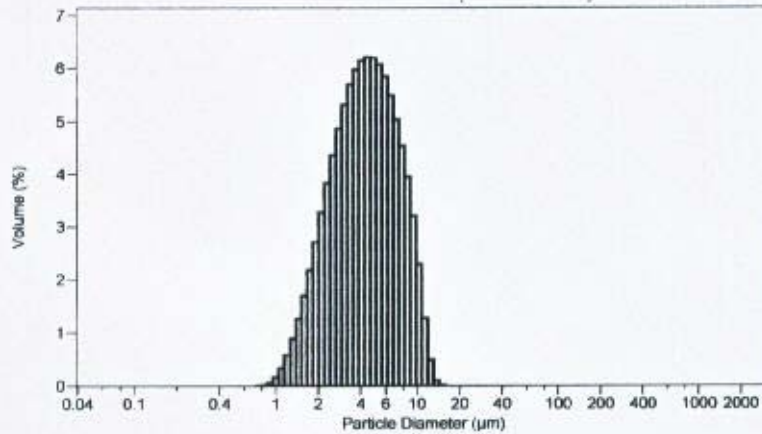

Volume:	100%	S.D.:	2.451 µm	Number:	100%	S.D.:	1.124 µm
Mean:	4.788 µm	Variance:	6.005 µm ²	Mean:	2.124 µm	Variance:	1.262 µm ²
Median:	4.285 µm	Skewness:	0.763 Right skewed	Median:	1.807 µm	Skewness:	2.297 Right skewed
Mean/Median Ratio:	1.117	Kurtosis:	0.057 Leptokurtic	Mean/Median Ratio:	1.175	Kurtosis:	8.150 Leptokurtic
Mode:	4.443 µm			Mode:	1.592 µm		
% >	1	50	90	% >	1	50	90
µm	11.49	8.411	4.288	µm	6.451	3.484	1.807
			2.019				1.141
			1.236				0.907